

2 Instrument Overview

The core of the LZ experiment is a two-phase xenon (Xe) time projection chamber (TPC) containing about 7 fully active tonnes of liquid Xe (LXe). Scattering events in LXe create both a prompt scintillation signal (S1) and free electrons. Various electric fields are employed to drift the electrons to the liquid surface, extract them into the gas phase above, and accelerate them to create a proportional scintillation signal (S2). Both signals are measured by arrays of photomultiplier tubes (PMTs) above and below the central region. The difference in time of arrival between the signals measures the position of the event in z , while the x,y position is determined from the pattern of S2 light in the top PMT array. Events with an S2 signal but no S1 are also recorded. A 3-D model of the LZ detector located in a water tank is shown in Figure 2.1. The water tank is located at the 4,850-foot level (4850L) of the Sanford Underground Research Facility (SURF). The heart of the LZ detector (including the inner titanium [Ti] cryostat) will be assembled on the surface at SURF, lowered in the Yates shaft to the 4850L of SURF, and deployed in the existing water tank in the Davis Cavern (where LUX is currently located). The principal parameters of the LZ experiment are given in Table 2.1, along with the proposed Work Breakdown Structure (WBS) for the LZ Project.

The LZ design is enhanced by several added capabilities beyond the successfully demonstrated LUX and ZEPLIN designs. The most important addition is a hermetic liquid organic scintillator (gadolinium-loaded linear alkyl benzene [LAB]) outer detector, which surrounds the central cryostat vessels and TPC. The outer detector and the active Xe “skin” layer operate as an integrated veto system, which has several benefits. The first is rejecting gammas and neutrons generated internally (e.g., in the PMTs) that scatter a single time in the fully active region and would otherwise escape without detection; this could mimic a weakly interacting massive particle (WIMP) signal. As these internally generated backgrounds interact primarily at the outer regions of the detector, the veto thus allows an increase in the fiducial volume.

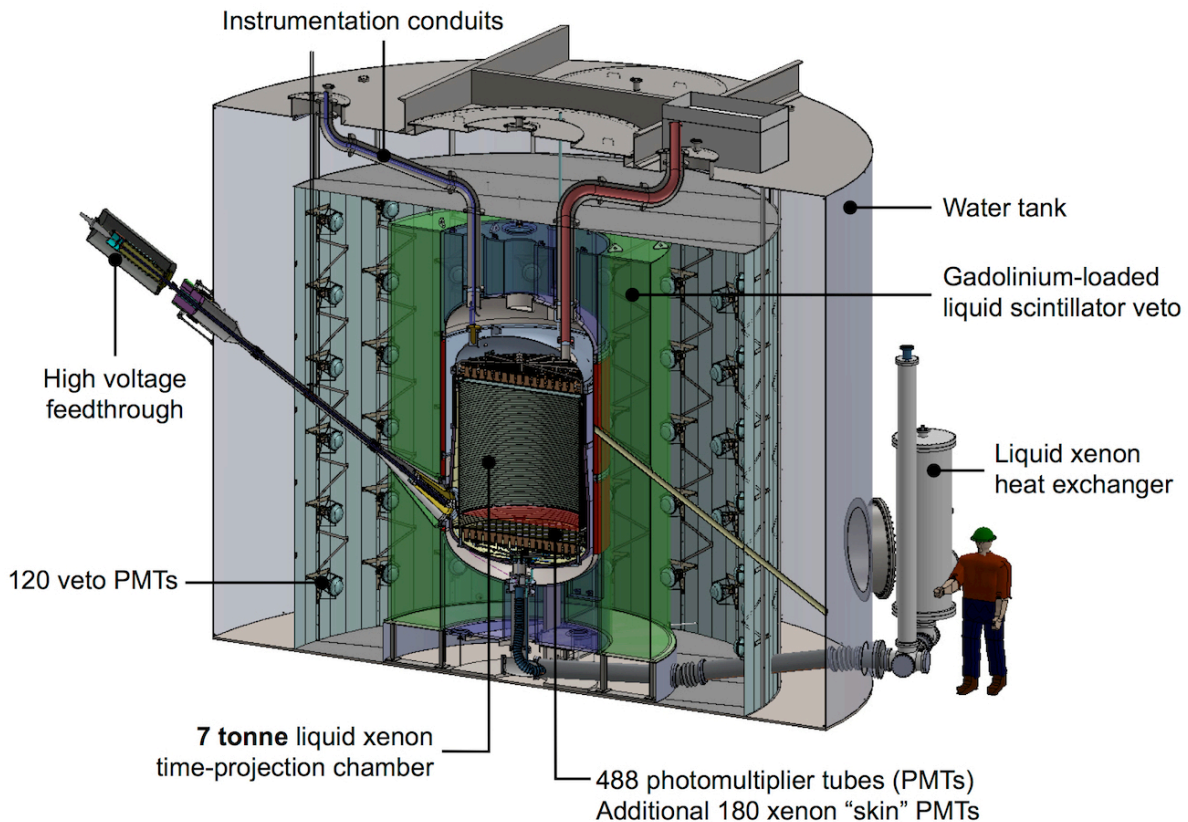


Figure 2.1. LZ detector concept.

Table 2.1 Work Breakdown Structure (WBS) and principal parameters of the LZ detector.

WBS	Description	Quantity
1.1	Xenon Procurement	
	Approximate total mass	10 tonnes
	Mass inside TPC active region	7 tonnes
	Approximate fiducial mass	5.6 tonnes
1.2	Cryostat	
	Inner cryostat — inside diameter (tapered), height, wall thickness	1.58–1.66 m, 2.52 m, 8 mm
	Outer cryostat — inside diameter, height, wall thickness	1.83 m, 3.09 m, 8 mm
	Approximate cryostat weights — inner, outer	0.74 tonne, 1.09 tonne
1.3	Cryogenic System	
	Cooling power	1 kW @ 80 K
	Input electrical power	11 kW
1.4	Xenon Purification	
	Krypton content	<0.015 ppt (g/g)
	²²² Rn content in active Xe	<0.67 mBq
	Recirculation rate	500 slpm
	Electron lifetime	>0.75 ms
	Charge attenuation length	>1.5 m
1.5	Xenon Detector	
	Top (Bottom) TPC 3-inch PMT array	247 (241), 488 total tubes
	“Side skin readout” and “bottom” 1-inch PMT	60 top skin, 60 bottom skin, 60 bottom
	Nominal (Design) cathode operating voltage	100 (200) kV
	Reverse field region (cathode to bottom tube shield)	0.146 m
	TPC height (cathode to gate grid)	1.456 m
	TPC effective diameter	1.456 m
1.6	Outer Detector System	
	Weight of Gd-loaded LAB scintillator	20.8 tonnes
	Number of acrylic vessels, total acrylic mass	9 vessels, 4 tonnes
	Number of 8-inch PMTs	120
	Minimum thickness of scintillator	0.61 m
	Diameter of water tank	7.62 m
	Height of water tank	5.92 m
	Approximate weight of water	228 tonnes
1.7	Calibration System	
	Number of source (γ , n) calibration tubes	3
	Other calibration tools	^{83m} Kr, n-generator, tritiated CH ₄ , ³⁷ Ar
1.8	Electronics, DAQ, Controls, and Computing	
	Trigger rate (all energies, 0-40 keV)	40 Hz, 0.4 Hz
	Average event size (noncalibration, uncompressed)	0.2–1.0 MB
	Data volume per year	350–850 TB
1.9	Integration and Installation	
1.10	Cleanliness and Screening	
1.11	Offline Computing	
1.12	Project Management	

Additionally, this direct vetoing is an important means of risk mitigation against one of the detector components (e.g., the cryostat materials or the PMTs) having a higher-than-expected background. A second benefit of the outer detector is that the combination of outer detector and segmented Xe detector will form a nearly hermetic detection system for all internal radioactivity. This will not only directly measure the internal backgrounds with an unprecedented level of detail and completeness, but also provide a similarly dramatic improvement in our understanding of the detector's response to those backgrounds.

The design of this scintillator veto is informed by proven designs of other experiments. As shown in Figure 2.1, the liquid scintillator volume is confined in a segmented, clear acrylic housing encapsulating the Ti cryostat of the central LZ detector. PMTs mounted on ladders in the outer water shield simultaneously view the light from both the scintillator and inner water volumes.

An important enhancement beyond LUX is the treatment of the “skin” layer of LXe located between the PTFE (polytetrafluoroethylene, or Teflon[®]) structure that surrounds the fully active region and the cryostat wall, as well as the region beneath the bottom PMT array. A skin of some (~few cm) thickness is difficult to avoid given the TPC geometry, the need for high-voltage standoff, and the strong mismatch in thermal expansion between the PTFE panels and Ti vessels. The skin readout alone has a limited veto efficiency, but has sufficient gamma-stopping power to augment the scintillator veto. The combination of skin readout and outer detector creates a highly efficient integrated veto system. Scintillation light from the skin region is observed by a sparse PMT array dedicated to this region. Thin (6-mm) PTFE panels are attached to the inner cryostat wall to enhance light collection in this region.

For detector calibration, neutron and gamma-ray sources will be brought next to the wall of the inner cryostat via an array of three source tubes that penetrate the water and organic scintillator. The principal calibrations, metastable krypton and tritiated methane, will be introduced directly into the LXe via the Xe gas-handling system to allow in situ calibration, which has been demonstrated in LUX. An external neutron generator will also be employed, as has also been the case for LUX.

Another key determinant of the sensitivity of the experiment is the level of discrimination of electron recoil (ER) backgrounds from nuclear recoils (NRs). This depends on the electric field established in the TPC. The nominal operating voltage (cathode-to-anode) is 100 kV but all components will be designed to a voltage of 200 kV to have sufficient operating margin.

The LZ TPC detector will employ Hamamatsu R11410-20 3-inch-diameter PMTs with a demonstrated low level of radioactive contamination and high quantum efficiency. Care will be taken in the design of the highly reflective PTFE TPC structure to isolate light produced in the central volume from the skin region, and vice-versa. Additional 1-inch PMTs will be utilized in the skin region.

As in LUX, LZ will employ an array of liquid nitrogen (LN)-cooled thermosyphons to control the detector temperature and minimize thermal gradients. The baseline purification system is a scaled-up version of the LUX room-temperature gas-phase purification system, and will exploit the liquid/gas heat-exchanger technology developed for LUX to minimize LN consumption. Krypton will be removed from the gaseous Xe using scaled-up techniques already demonstrated successfully for LUX.

The electronics front-end, trigger and data acquisition, and slow controls are based on the LUX experience but will be significantly expanded and improved. Software and computing systems for LZ are based on the successful operation of LUX and analysis of LUX data but will be substantially augmented to accommodate the larger LZ data volume. LZ data will be buffered locally at SURF and then transmitted to primary data storage that will be mirrored in the United States and the UK. The simulation of the LZ detector and its response is already well advanced, and the results are given in other chapters of this *Conceptual Design Report*.

Components of LZ will be manufactured and brought to SURF. Assembly of the Xe detector and the inner cryostat will occur in a dedicated clean room at SURF that includes air handling to remove radon.

The inner cryostat with the Xe detector will be lowered as a unit down the Yates shaft and transported to the Davis Cavern water tank. All other components will be staged at SURF, lowered via the Yates shaft, and similarly transported. This includes the segmented acrylic vessels for the outer detector system and other large components.